


Breast Reconstruction, Mammoplasty & Mastectomy Incision Pathway

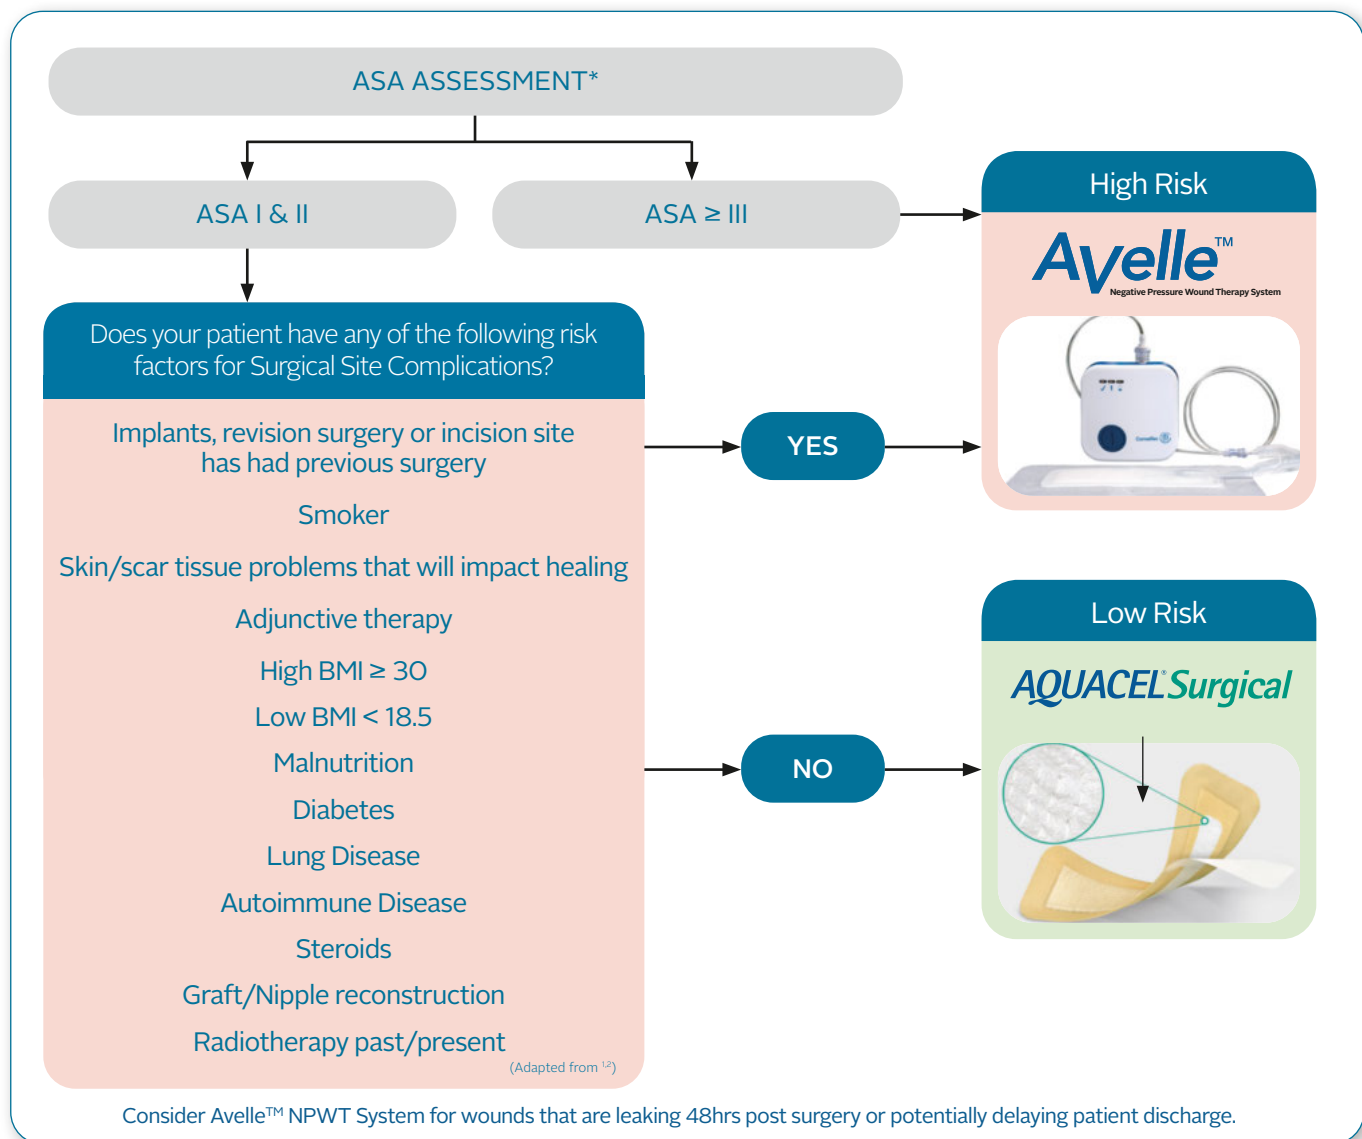

Ordering information for Avelle™ NPWT System and AQUACEL® Surgical

Avelle™ NPWT System

Description	Product Code	Pack Size	NHS Code
Avelle™ Pump	421551	1	ELZ853
Pump Carry Bag	446650	1	ELZ875
16 x 16 cm	421552	5	ELZ857
16 x 21 cm	421553	5	ELZ856
12 x 21 cm	421554	5	ELZ855
12 x 31 cm	421555	5	ELZ854
12 x 41 cm	422155	5	ELZ965
21 x 26 cm	422156	5	ELZ981
26 x 26 cm	422157	5	ELZ982
HydroColloid Sealing Strips	422308	10	ELB000

AQUACEL® Ag Surgical

Description	Product Code	Pack Size	NHS Code
9 cm x 10 cm	412009	10	ELY341
9 cm x 15 cm	412010	10	ELY342
9 cm x 25 cm	412011	10	ELY343
9 cm x 30 cm	420670	10	ELY403
9 cm x 35 cm	412012	10	ELY344

AQUACEL® Surgical

Description	Product Code	Pack Size	NHS Code
9 x 10 cm	412017	10	ELY323
9 x 15 cm	412018	10	ELY324
9 x 25 cm	412019	10	ELY325
9 x 30 cm	420669	10	ELY402
9 x 35 cm	412020	10	ELY326

ConvaTec representative: **First Name Last Name**
Tel: 22222 22222 Email: **First Name.Last Name@convatec.com**

For more information or assistance please contact:
0800 289 738 (UK) or 1800 946 938 (ROI)




*The American Society of Anesthesiologists physical classification system designed to assess the fitness of patients before surgery.

Always consult your hospital/institution policy on incision management. Assessment of patients for their surgical risk and decisions regarding their subsequent incision management is at the discretion of the clinician. Patients who present as low/medium risk may still be suitable for closed incision NPWT management. Patients may present risk factors for surgical site complications, but NPWT may not be acceptable for patient.

1. World Union of Wound Healing Societies (WUWHS) Consensus Document. Closed surgical incision management: understanding the role of NPWT. Wounds International, 2016.
2. National Institute for Health and Clinical Excellence. Surgical Site Infection Guideline. 2008.

®/TM indicates a trademark of ConvaTec Inc. ConvaTec is an authorised user. ©2020 ConvaTec Inc. AP-021206-GB

Cardiothoracic Incision Pathway

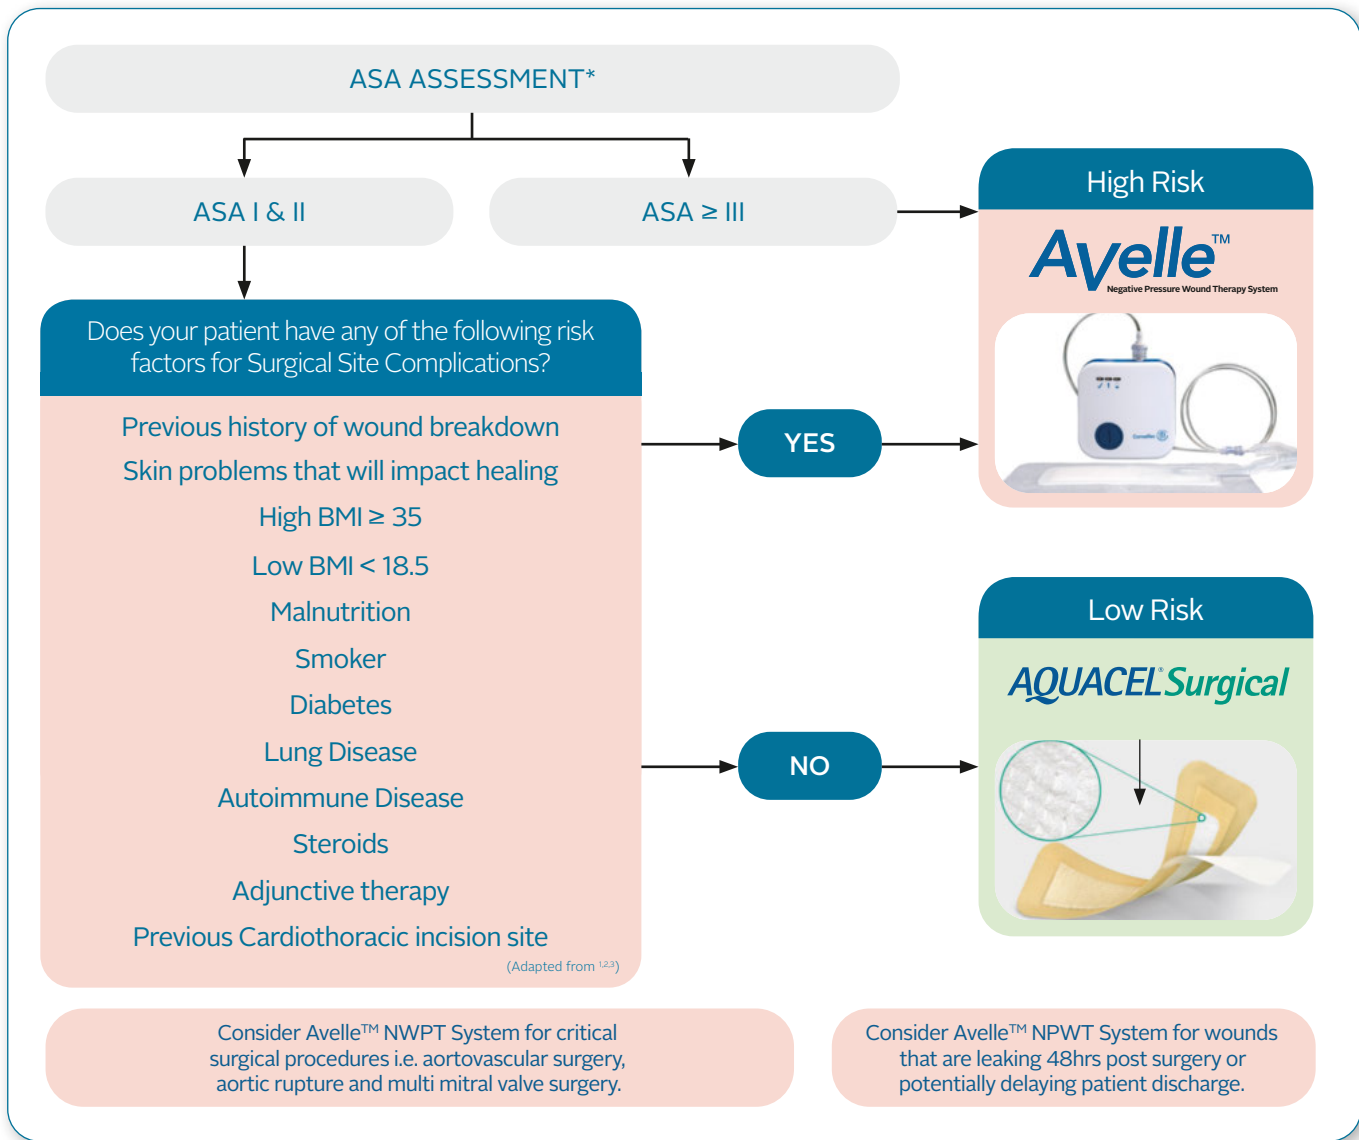

Ordering information for Avelle™ NPWT System and AQUACEL® Surgical

Avelle™ NPWT System				AQUACEL® Ag Surgical				AQUACEL® Surgical			
Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code
Avelle™ Pump	421551	1	ELZ853	9 cm x 10 cm	412009	10	ELY341	9 x 10 cm	412017	10	ELY323
Pump Carry Bag	446650	1	ELZ875	9 cm x 15 cm	412010	10	ELY342	9 x 15 cm	412018	10	ELY324
16 x 16 cm	421552	5	ELZ857	9 cm x 25 cm	412011	10	ELY343	9 x 25 cm	412019	10	ELY325
16 x 21 cm	421553	5	ELZ856	9 cm x 30 cm	420670	10	ELY403	9 x 30 cm	420669	10	ELY402
12 x 21 cm	421554	5	ELZ855	9 cm x 35 cm	412012	10	ELY344	9 x 35 cm	412020	10	ELY326
12 x 31 cm	421555	5	ELZ854								
12 x 41 cm	422155	5	ELZ965								
21 x 26 cm	422156	5	ELZ981								
26 x 26 cm	422157	5	ELZ982								
HydroColloid Sealing Strips	422308	10	ELB000								

ConvaTec representative: **First Name Last Name**
Tel: 22222 22222 Email: **First Name.Last Name@convatec.com**

For more information or assistance please contact:
0800 289 738 (UK) or 1800 946 938 (ROI)




*The American Society of Anesthesiologists physical classification system designed to assess the fitness of patients before surgery.

Always consult your hospital/institution policy on incision management. Assessment of patients for their surgical risk and decisions regarding their subsequent incision management is at the discretion of the clinician. Patients who present as low/medium risk may still be suitable for closed incision NPWT management. Patients may present risk factors for surgical site complications, but NPWT may not be acceptable for patient.

1. World Union of Wound Healing Societies (WUWHs) Consensus Document. Closed surgical incision management: understanding the role of NPWT. Wounds International, 2016.
2. National Institute for Health and Clinical Excellence. Surgical Site Infection Guideline. 2008.
3. Cardiothoracic Surgery GIRFT Programme National Specialty Report David Richens, March 2018.

Gynaecology

Incision Pathway

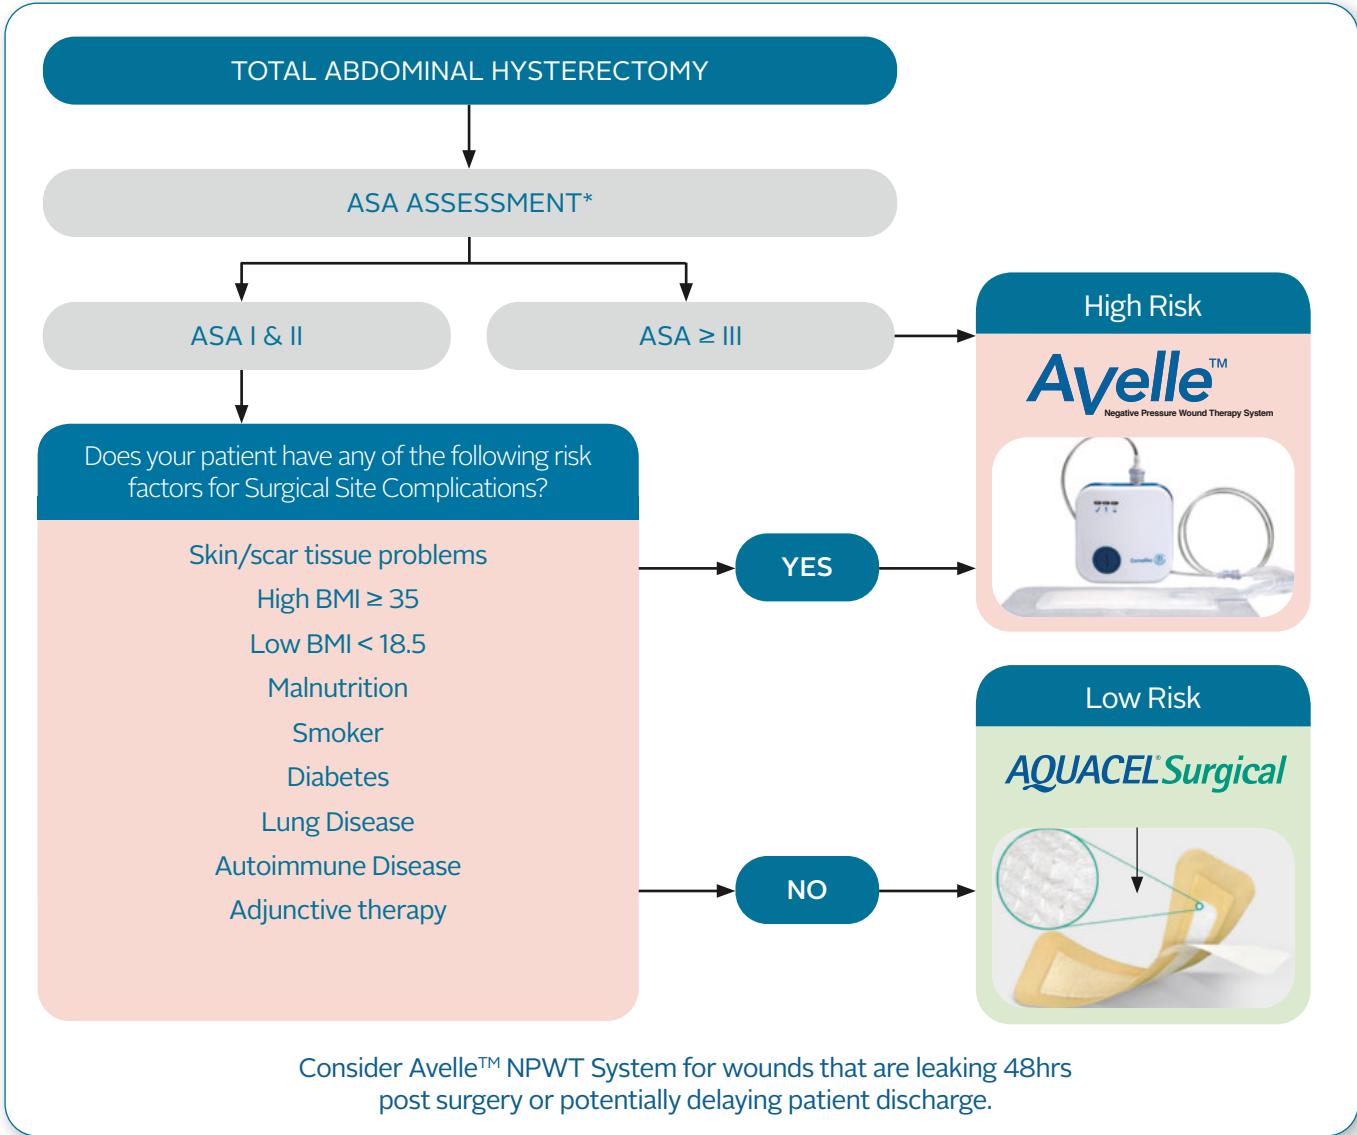

Ordering information for Avelle™ NPWT System and AQUACEL® Surgical

Avelle™ NPWT System				AQUACEL® Ag Surgical				AQUACEL® Surgical			
Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code
Avelle™ Pump	421551	1	ELZ853	9 cm x 10 cm	412009	10	ELY341	9 x 10 cm	412017	10	ELY323
Pump Carry Bag	446650	1	ELZ875	9 cm x 15 cm	412010	10	ELY342	9 x 15 cm	412018	10	ELY324
16 x 16 cm	421552	5	ELZ857	9 cm x 25 cm	412011	10	ELY343	9 x 25 cm	412019	10	ELY325
16 x 21 cm	421553	5	ELZ856	9 cm x 30 cm	420670	10	ELY403	9 x 30 cm	420669	10	ELY402
12 x 21 cm	421554	5	ELZ855	9 cm x 35 cm	412012	10	ELY344	9 x 35 cm	412020	10	ELY326
12 x 31 cm	421555	5	ELZ854								
12 x 41 cm	422155	5	ELZ965								
21 x 26 cm	422156	5	ELZ981								
26 x 26 cm	422157	5	ELZ982								
HydroColloid Sealing Strips	422308	10	ELB000								

ConvaTec representative: **First Name Last Name**
 Tel: 22222 22222 Email: **First Name.Last Name@convatec.com**

For more information or assistance please contact:
0800 289 738 (UK) or 1800 946 938 (ROI)




*The American Society of Anesthesiologists physical classification system designed to assess the fitness of patients before surgery.

Always consult your hospital/institution policy on incision management. Assessment of patients for their surgical risk and decisions regarding their subsequent incision management is at the discretion of the clinician. Patients who present as low/medium risk may still be suitable for closed incision NPWT management. Patients may present risk factors for surgical site complications, but NPWT may not be acceptable for patient.

1. World Union of Wound Healing Societies (WUWHS) Consensus Document. Closed surgical incision management: understanding the role of NPWT. Wounds International, 2016.
 2. National Institute for Health and Clinical Excellence. Surgical Site Infection Guideline. 2008.

©/TM indicates a trademark of ConvaTec Inc. ConvaTec is an authorised user. ©2020 ConvaTec Inc. AP-021206-GB

Laparotomy Incision Pathway

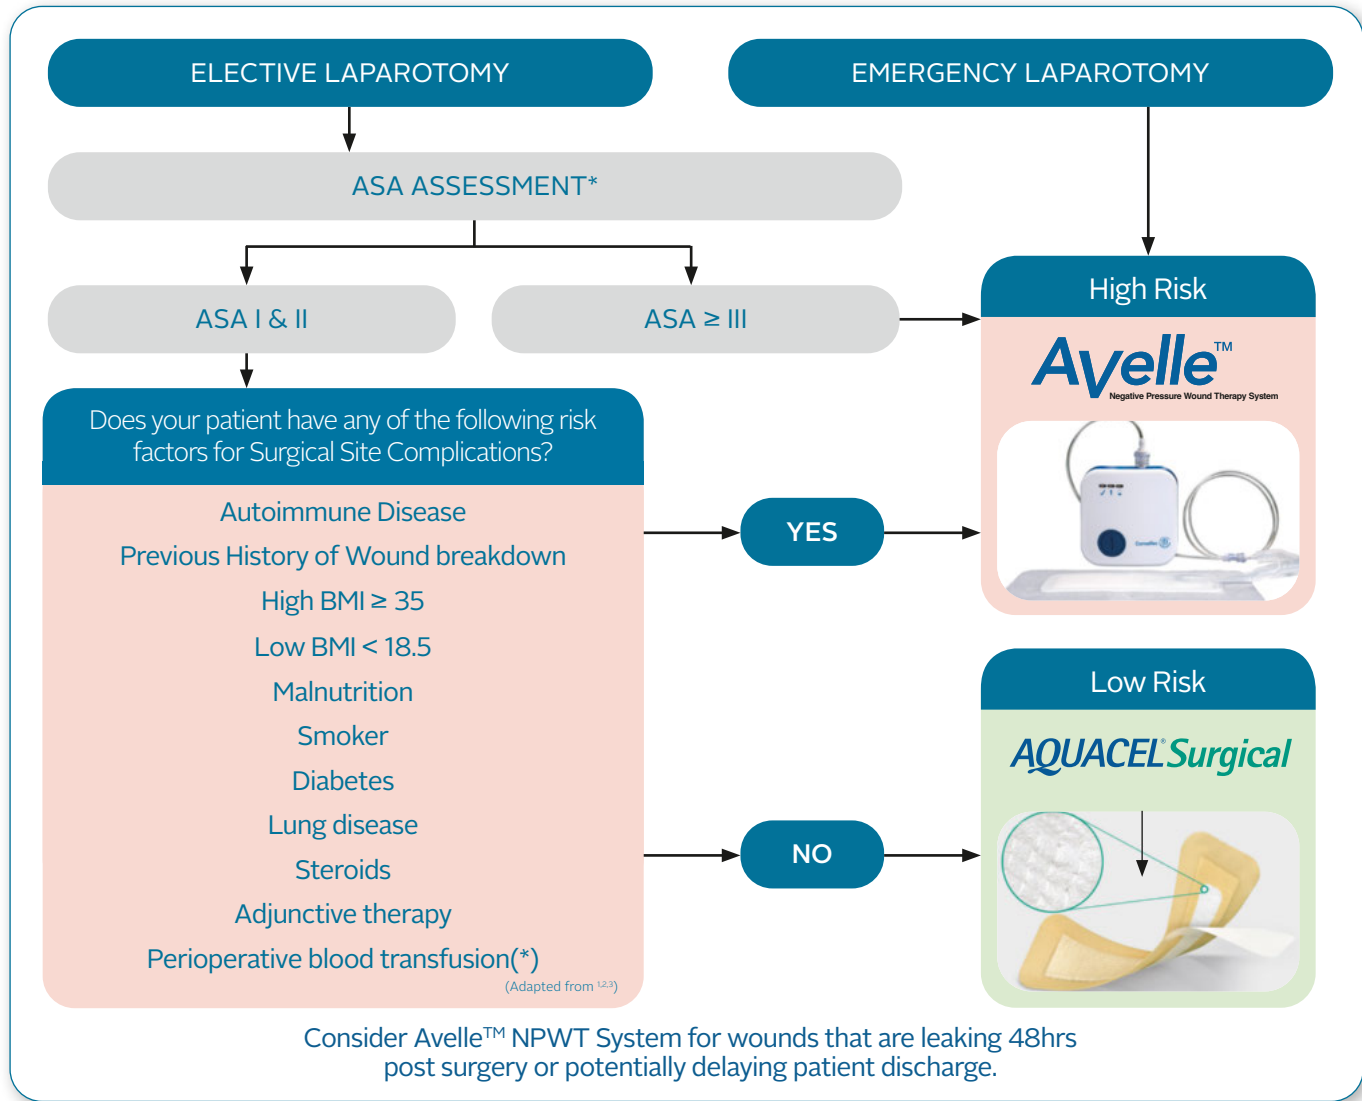

Ordering information for Avelle™ NPWT System and AQUACEL® Surgical

Avelle™ NPWT System				AQUACEL® Ag Surgical				AQUACEL® Surgical			
Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code
Avelle™ Pump	421551	1	ELZ853	9 cm x 10 cm	412009	10	ELY341	9 x 10 cm	412017	10	ELY323
Pump Carry Bag	446650	1	ELZ875	9 cm x 15 cm	412010	10	ELY342	9 x 15 cm	412018	10	ELY324
16 x 16 cm	421552	5	ELZ857	9 cm x 25 cm	412011	10	ELY343	9 x 25 cm	412019	10	ELY325
16 x 21 cm	421553	5	ELZ856	9 cm x 30 cm	420670	10	ELY403	9 x 30 cm	420669	10	ELY402
12 x 21 cm	421554	5	ELZ855	9 cm x 35 cm	412012	10	ELY344	9 x 35 cm	412020	10	ELY326
12 x 31 cm	421555	5	ELZ854								
12 x 41 cm	422155	5	ELZ965								
21 x 26 cm	422156	5	ELZ981								
26 x 26 cm	422157	5	ELZ982								
HydroColloid Sealing Strips	422308	10	ELB000								

ConvaTec representative: **First Name Last Name**
 Tel: 22222 22222 Email: **First Name.Last Name@convatec.com**

For more information or assistance please contact:
0800 289 738 (UK) or 1800 946 938 (ROI)



*The American Society of Anesthesiologists physical classification system designed to assess the fitness of patients before surgery.

Always consult your hospital/institution policy on incision management. Assessment of patients for their surgical risk and decisions regarding their subsequent incision management is at the discretion of the clinician. Patients who present as low/medium risk may still be suitable for closed incision NPWT management. Patients may present risk factors for surgical site complications, but NPWT may not be acceptable for patient.

1. World Union of Wound Healing Societies (WUWHS) Consensus Document. Closed surgical incision management: understanding the role of NPWT. Wounds International, 2016.

2. National Institute for Health and Clinical Excellence. Surgical Site Infection Guideline. 2008.

3. Surgical Site Infection Following Bowel Surgery - A Retrospective Analysis of 1446 Patients. J. Matthias Walz, MD; Craig A. Paterson, MD; Jeanne M. Seligowski, RN; et al October 1, 2006

Perioperative Allogeneic Blood Transfusion Is Associated With Surgical Site Infection After Abdominoperineal Resection—a Space for the Implementation of Patient Blood Management Strategies; Int Surg. 2015 May; 100(5): 797–804.

Obstetrics

Incision Pathway



Caesarean Section

Does your patient have any of the following risk factors for Surgical Site Complications?

- Previous Caesarean Section incision site complications
- High BMI ≥ 35
- Low BMI < 18.5
- Diabetes Type 1 & Type 2

(Adapted from ^{1,2})

YES

High Risk

Avelle™
Negative Pressure Wound Therapy System

NO

Low Risk

AQUACEL® Surgical

Consider **Avelle™ NPWT System** for

- Patients with gestational diabetes
- Smokers
- Patients with increased risk of Venous Thromboembolism event (VTE)
- Wounds that are leaking 48hrs post surgery

Ordering information for Avelle™ NPWT System and AQUACEL® Surgical

Avelle™ NPWT System				AQUACEL® Ag Surgical				AQUACEL® Surgical			
Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code
Avelle™ Pump	421551	1	ELZ853	9 cm x 10 cm	412009	10	ELY341	9 x 10 cm	412017	10	ELY323
Pump Carry Bag	446650	1	ELZ875	9 cm x 15 cm	412010	10	ELY342	9 x 15 cm	412018	10	ELY324
16 x 16 cm	421552	5	ELZ857	9 cm x 25 cm	412011	10	ELY343	9 x 25 cm	412019	10	ELY325
16 x 21 cm	421553	5	ELZ856	9 cm x 30 cm	420670	10	ELY403	9 x 30 cm	420669	10	ELY402
12 x 21 cm	421554	5	ELZ855	9 cm x 35 cm	412012	10	ELY344	9 x 35 cm	412020	10	ELY326
12 x 31 cm	421555	5	ELZ854								
12 x 41 cm	422155	5	ELZ965								
21 x 26 cm	422156	5	ELZ981								
26 x 26 cm	422157	5	ELZ982								
HydroColloid Sealing Strips	422308	10	ELB000								

ConvaTec representative: **First Name Last Name**
 Tel: 22222 22222 Email: **First Name.Last Name@convatec.com**

For more information or assistance please contact:
0800 289 738 (UK) or 1800 946 938 (ROI)




*The American Society of Anesthesiologists physical classification system designed to assess the fitness of patients before surgery.

Always consult your hospital/institution policy on incision management. Assessment of patients for their surgical risk and decisions regarding their subsequent incision management is at the discretion of the clinician. Patients who present as low/medium risk may still be suitable for closed incision NPWT management. Patients may present risk factors for surgical site complications, but NPWT may not be acceptable for patient.

1. World Union of Wound Healing Societies (WUWHS) Consensus Document. Closed surgical incision management: understanding the role of NPWT. Wounds International, 2016.
 2. National Institute for Health and Clinical Excellence. Surgical Site Infection Guideline. 2008.

Trauma and Orthopaedic Incision Pathway

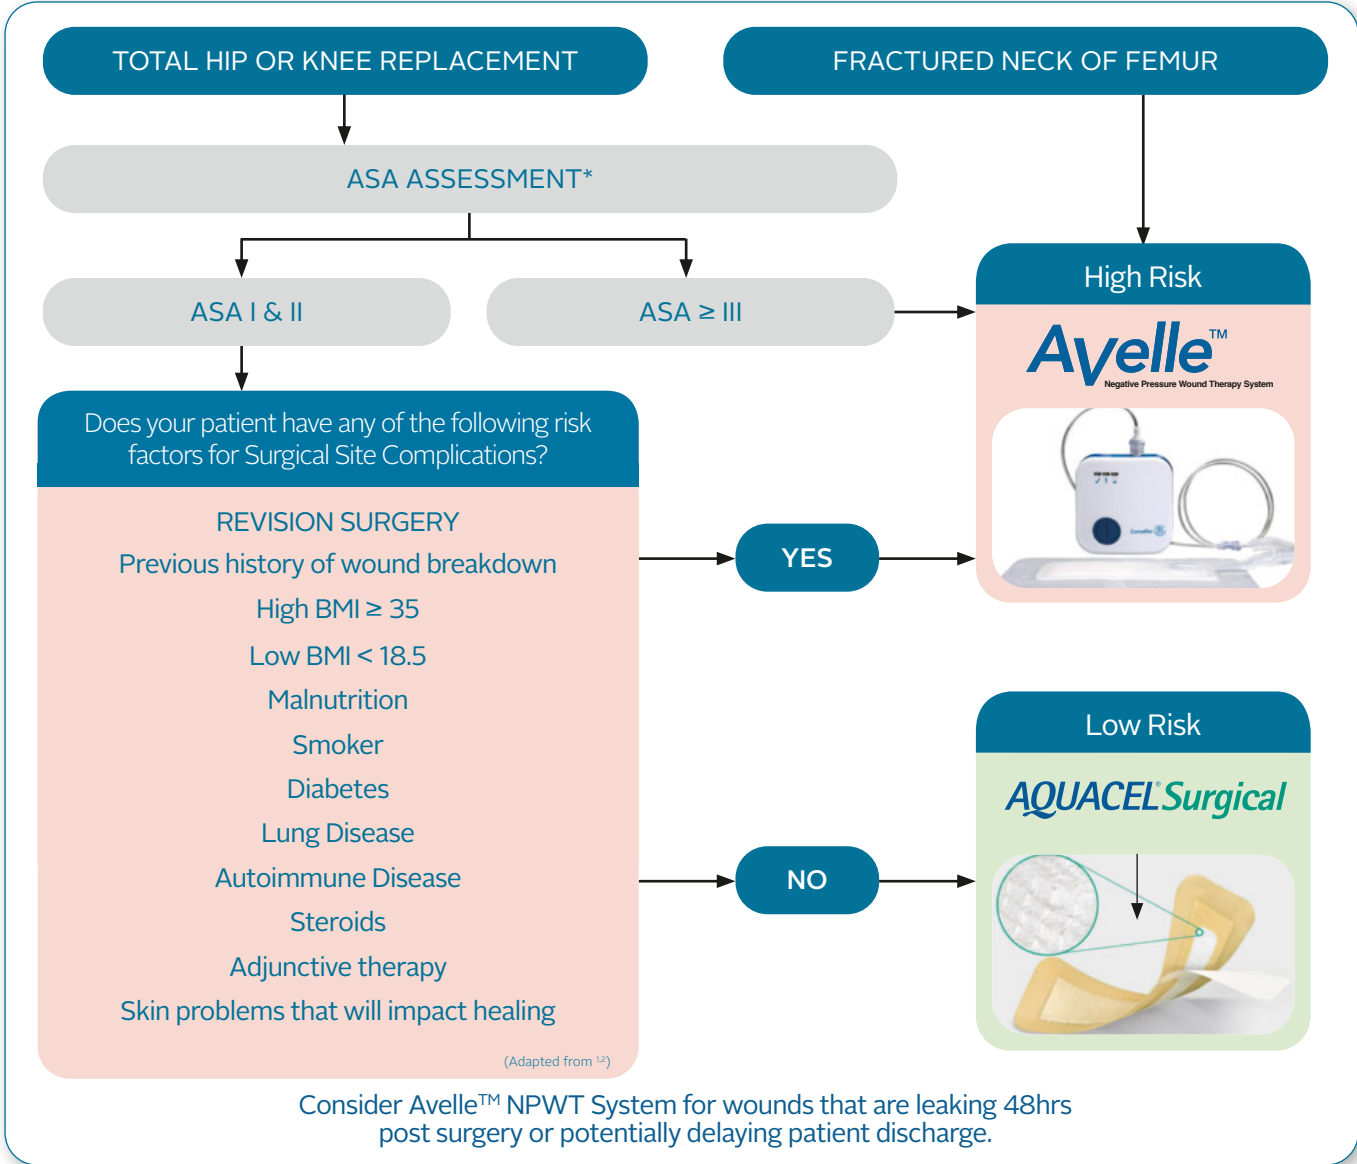

Ordering information for Avelle™ NPWT System and AQUACEL® Surgical

Avelle™ NPWT System				AQUACEL® Ag Surgical				AQUACEL® Surgical			
Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code	Description	Product Code	Pack Size	NHS Code
Avelle™ Pump	421551	1	ELZ853	9 cm x 10 cm	412009	10	ELY341	9 x 10 cm	412017	10	ELY323
Pump Carry Bag	446650	1	ELZ875	9 cm x 15 cm	412010	10	ELY342	9 x 15 cm	412018	10	ELY324
16 x 16 cm	421552	5	ELZ857	9 cm x 25 cm	412011	10	ELY343	9 x 25 cm	412019	10	ELY325
16 x 21 cm	421553	5	ELZ856	9 cm x 30 cm	420670	10	ELY403	9 x 30 cm	420669	10	ELY402
12 x 21 cm	421554	5	ELZ855	9 cm x 35 cm	412012	10	ELY344	9 x 35 cm	412020	10	ELY326
12 x 31 cm	421555	5	ELZ854								
12 x 41 cm	422155	5	ELZ965								
21 x 26 cm	422156	5	ELZ981								
26 x 26 cm	422157	5	ELZ982								
HydroColloid Sealing Strips	422308	10	ELB000								

ConvaTec representative: **First Name Last Name**
 Tel: 22222 22222 Email: **First Name.Last Name@convatec.com**

For more information or assistance please contact:
0800 289 738 (UK) or 1800 946 938 (ROI)



*The American Society of Anesthesiologists physical classification system designed to assess the fitness of patients before surgery.
 Always consult your hospital/institution policy on incision management. Assessment of patients for their surgical risk and decisions regarding their subsequent incision management is at the discretion of the clinician. Patients who present as low/medium risk may still be suitable for closed incision NPWT management. Patients may present risk factors for surgical site complications, but NPWT may not be acceptable for patient.
 1. World Union of Wound Healing Societies (WUWHS) Consensus Document. Closed surgical incision management: understanding the role of NPWT. Wounds International, 2016.
 2. National Institute for Health and Clinical Excellence. Surgical Site Infection Guideline. 2008.
 ®/TM indicates a trademark of ConvaTec Inc. ConvaTec is an authorised user. ©2020 ConvaTec Inc. AP-021206-GB